



BioHorizons External Impression Technique Guide



BIOHORIZONS[®]
SCIENCE • INNOVATION • SERVICE

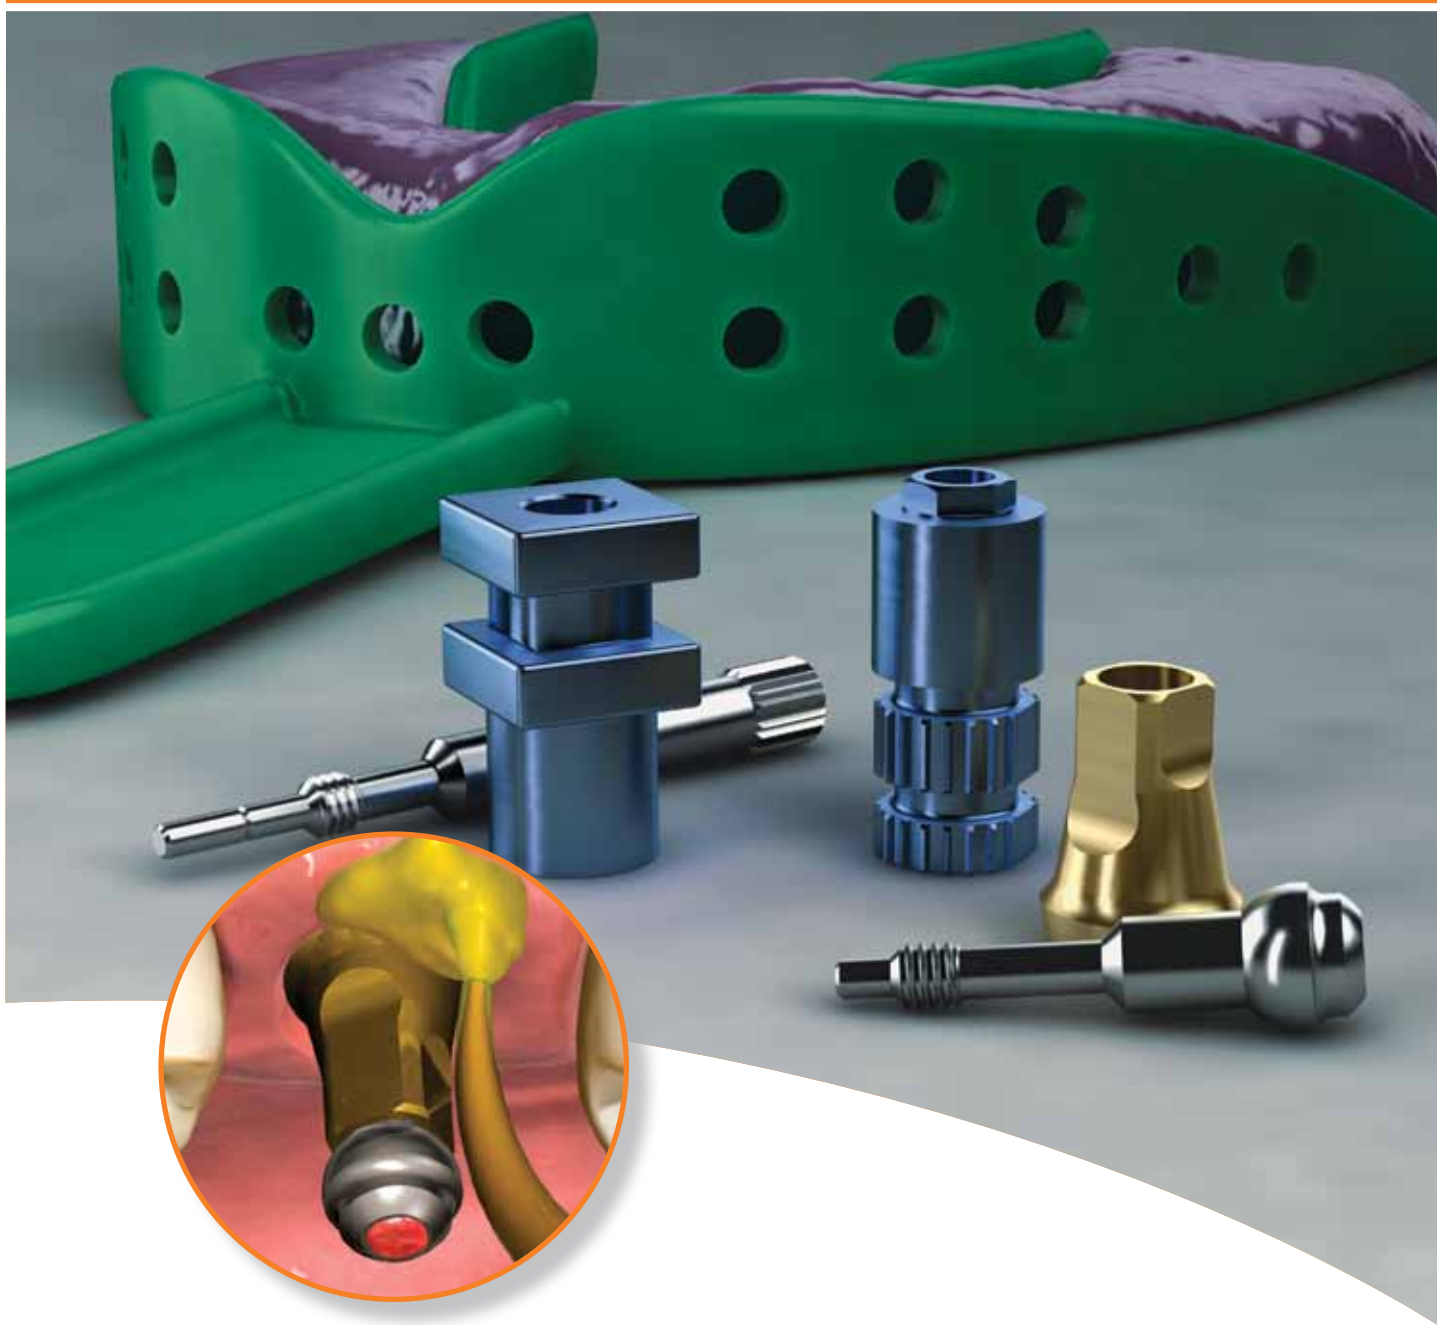



INDIRECT TRANSFER WITH THE 3INONE ABUTMENT / BALL-TOP SCREW

Procedure Objective: Make an impression for fabrication of a working cast utilizing a closed-tray, indirect transfer method when a flared emergence Healing Abutment was used. The procedure creates a cast that represents the exact position of the implant as well as the orientation of the external hex.

1. Remove Healing Abutment



Remove the flared emergence Healing Abutment with the .050" (1.25mm) Hex Driver. Confirm that the implant's prosthetic platform is free of bone debris or soft tissue.

2. Place Transfer Coping



Seat the 3inOne Abutment and secure it with a Ball-top Screw (hand-tighten).

If practical, orient the long flat side of the abutment to the facial for easier indexing.

Radiographically verify correct seating of the abutment.

3. Block out hex hole



Block out the hex-hole on top of the Ball-top Screw with a material of choice.

4. Make full-arch impression



Syringe a light-body elastomeric impression material around the coping assembly. Record the full arch impression using the closed tray loaded with heavier body impression material.


Remove the coping assembly after the tray has been removed. Replace the Healing Abutment immediately to prevent soft tissue collapse.

5. Assemble coping and analog



Use the Ball-top Screw to assemble the 3inOne Abutment with the corresponding Implant Analog.

6. Index coping into impression

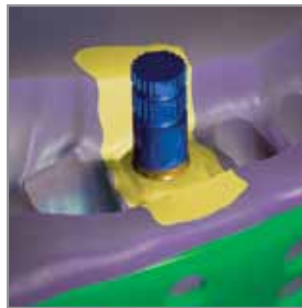

Insert the coping assembly into the corresponding location in the impression, ensuring that the long flat of the abutment aligns with the corresponding indice within the impression.

Send the impression, coping/analog assembly, abutment screw, bite registration and opposing model to the lab.

Lab Steps



Send to Lab

- Impression
- 3inOne/Ball-top Screw combo
- Abutment Screw (comes with 3inOne)
- Implant Analog
- Bite Registration
- Opposing model or impression
- Shade selection

7. Create soft tissue model




A soft tissue replica material is recommended around the analog. Verify analog seating and apply lubricant where soft tissue replica material is to be applied.

8. Fabricate working cast



Fabricate a working cast. Articulate according to standard laboratory procedures.



DIRECT PICK-UP

Procedure Objective: Make an impression for fabrication of a working cast utilizing an open-tray, direct pick-up method. The procedure creates a cast that represents the exact position of the implant. Hex orientation may be registered (single-unit) or bypassed (multiple-units) depending on the coping selected.

1. Remove Healing Abutment



Remove the Healing Abutment with the .050" (1.25mm) Hex Driver. Confirm that the implant prosthetic platform is free of bone debris or soft tissue.

2. Place Pick-up Coping



Place the appropriate diameter Direct Pick-up Coping (either hexed or non-hexed) on the implant body and retain with the corresponding coping screw (hand-tighten).

These screws feature a knurled top to aid in manual insertion, as well as a .050" (1.25mm) hex access hole for insertion with the Hex Driver.

Radiographically verify correct seating of the coping.

3. Verify screw/tray clearance



A stock impression tray may be modified for this procedure, or a custom tray may be fabricated using a tray material of choice. A window is cut out of the tray to allow clearance for the coping screw.


Try in the impression tray to verify that the coping screw protrudes through it without interference.

4. Make full-arch impression



Syringe a light-body elastomeric impression material around the coping assembly. Record the full arch impression with the tray loaded with heavier body impression material.


5. Remove impression tray from mouth

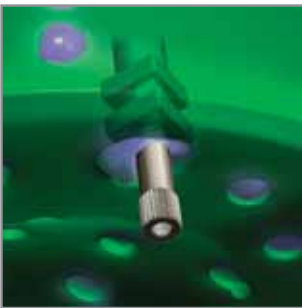

After the impression material has set, first remove the coping screw, and then remove the tray from the mouth. Verify that the impression material is completely adapted around the pick-up copings.

Replace the Healing Abutment immediately to prevent soft tissue collapse.

6. Attach analog to Pick-up Coping

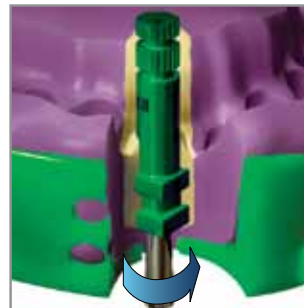

Assemble the appropriate diameter Implant Analog to the Direct Pick-up Coping with the coping screw.

Send the impression/coping assembly, bite registration and opposing model to the lab.

Lab Steps



Send to Lab

- Impression with coping inside
- Coping Screw
- Implant Analog
- Abutment and Screw (if selected)
- Bite Registration
- Opposing model or impression
- Shade selection

7. Create soft tissue model



A soft tissue replica material is recommended around the analog. Verify analog seating and apply lubricant where soft tissue replica material is to be applied.

8. Fabricate working cast



Fabricate a working cast. Articulate according to standard laboratory procedures.

BioHorizons USA

2300 Riverchase Center
Birmingham, AL 35244

Customer Care / Servicio al Cliente:
888-246-8338 or 205-967-7880

BioHorizons Canada

21 Amber Street, Unit # 6
Markham, Ontario L3R 4Z3

Customer Care / Service à la Clientèle:
866-468-8338 or / ou 905-944-1700

BioHorizons Spain

Serrano Anguita, 10
28004 Madrid, España

Atención al Cliente:
+34 91 713 10 84

BioHorizons UK

180 Dukes Ride
Crowthorne, Berkshire RG45 6DS

Customer Care:
+44 8700 620 550

BioHorizons Germany

Marktplatz 3
79199 Kirchzarten

Kunden Service:
+49 7661-909989-0

BioHorizons Australia

25-33 Allen Street
Waterloo NSW 2012

Customer Service:
+61 2 8399 1520

BioHorizons Mexico

Kelvin 8 Int. 303
Col. Anzures
C.P. 11590, Mexico, D.F.

Servicio al Cliente:
+52 55 5545 1297

BioHorizons Chile

Juan Esteban Montero 5944
Las Condes
Santiago, Chile

Atención al Cliente:
+56 2 475 7230

BioHorizons products are cleared for sale in the European Union under the EU Medical Device Directive 93/42/EEC. We are proud to be registered to ISO 13485:2003, the international quality management system standard for medical devices, which supports and maintains our product licences with Health Canada and in other markets around the globe.

© 2008 BioHorizons Implant Systems, Inc. All Rights Reserved. ML0207 REV B FEB 2008

w w w . b i o h o r i z o n s . c o m

